USB Digital Microscope






Table of Contents

Precauti	on	
Prepara	tion	4
	Standard accessories	4
•	Parts Names & Functions	
•	Computer System requirements	
•	Technical Specifications	
Install th	ne microscope	
	get focus	
Install th	e software in Windows	14
Start M	icroscope	15
	e functions	
•	Capture Photo	16
•	Capture Video	16
•	Timer	
Calibrati	on and Measurement	18
•	Calibration	18
•	Measurement	
•	Change Calibration	
•	Draw and text	
Software Interface Instructions		28
•	Main Interface Icons	
•	Main Menu	
•	Options	30
•	Capture	
•	Measurement Interface Instruction	
Instruction	ons for Mac software	
•	How to Install the Software	
	How to use MicroCapture Pro	

Welcome

Thank you for your choice of our product - it is a high-tech while easy to use Digital Microscope. With this unit you will see a unique and "bigger" world.

It's easy to zoom in on stamps, coins, paper currency, plants, insects, rocks and minerals, and so much more.

We recommend reading this manual first to get the best out of this unit.

1. Precaution


Before using The USB Digital Microscope, please ensure that you read and understand the safety precautions described below. Always ensure that the USB Digital Microscope is operated correctly.

- The Microscope is not waterproof, so keep it dry.
- Do not use it in a humid place like bathrooms. A dry environment will maintain its life to maximum.
- Use the Microscope only at -5°C-50°C.
- Sudden temperature change may form dew inside the Microscope like entering a warm room in cold winter. Put it inside a handbag or plastic bag to slow down temperature changes.
- Do not point Microscope lens to the sun or strong light for a long time. Powerful light may hurt the light-sensitive electronics.
- Avoid touching the lens.


- The white LEDs which illuminate the Microscope target field are very bright. Do not stare directly into these LEDs as it may damage your eyes.
- The clear plastic distance shell sometimes picks up dirt or toxic material from a microscopically observed surface. Be careful that this doesn't get in contact with the human skin. Always wash carefully or disinfect as needed.
- Do not unplug the Microscope from USB port when LEDs are on. This may cause information loss or circuit damage. Please always close MicroCapture Pro and then unplug the Microscope.

2. Preparation

Standard accessories

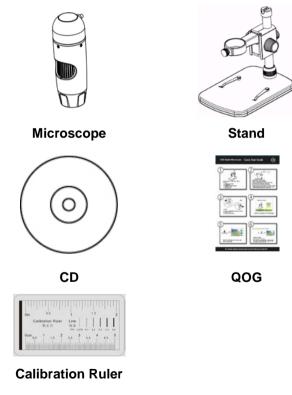

■ Parts Names & Functions

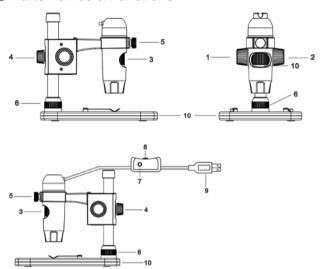

- 1. Wheel 1: move the microscope up and down
- 2. **Wheel 2:** lock or release the movement part that carries the microscope
- 3. Wheel 3: Focus adjustment wheel
- 4. Wheel 4: Fix the movement part on to the metal pole
- 5. Wheel 5: fix the microscope in the ring
- 6. Wheel 6: Fix the upper part on to the stage
- Snapshot button: take a snapshot (for Windows only)
- 8. LED dimmer: adjust the brightness of the LEDs
- 9. USB plug: USB connection
- 10. **Stage**

■ Computer System Requirements

11. Windows XP / VISTA / WIN7 / WIN8 & Mac 10.6~10.8.

12. P4 1.8 or above

13. RAM: 512M

14. Video Memory: 64M


15. USB port: 2.0 16. CD-ROM Drive

■ Technical Specifications

Image sensor	5 Mega Pixels (true resolution)	
	,	
Still capture resolution	2592x1944, 2048x1536, 1600x1200, 1280x960	
Video capture resolution	1280x960	
Focus Range	Manual focus from 0mm to 150mm	
Magnification Ratio	10x~300x	
Video format	AVI	
Photo format	JPEG	
Light source	8 LED (adjustable by control wheel)	
PC interface	USB2.0	
Power source	5V DC from USB port	
Operation system	Windows XP/Vista/Win7/ Win8/Mac 10.6~10.8	
OSD language	English, Deutsch, Spanish, Russian, Italian, French,	
	Portuguese, Dutch, Polish, Japanese, Korean, Chinese	
Bundle software	MicroCapture Pro	
Size	Microscope: 110mm (L) x 33mm (R)	
	Professional Stand: 165mm(L) x118mm(W)x12mm (H)	

3. Install the microscope

- 1) Take the microscope out from gift box gently; put the carriage stage on a flat surface.
- 2) Follow the below steps:

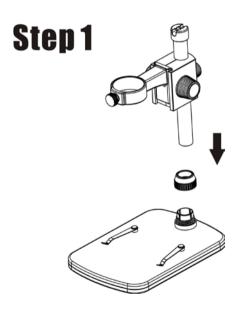

Put the metal pole through Wheel 6!



Put the metal pole into the female part of the stage!



Rotate Wheel 6 to fix the pole on the stage!




Put the microscope into the ring of the stand!



Rotate Wheel 5 clockwise to fix the microscope on the ring.

- Adjust the upper part of the stand to get a proper height.
- (2) Rotate Wheel 4 clockwise to fix the upper part.


Step 6




4. How to get focus



Rotate Wheel 1 to get a rough focus!



Rotate Wheel 3 to get a fine focus!



Rotate Wheel 2 to lock or release the movement!

5. Install the software in Windows

Insert the driver CD into CD-ROM Drive and this will automatically display the following interface:




- Install MicroCapture Pro Click Install MicroCapture Pro and the installation wizard will guide you through the whole process.
- 2) Full user's manual can be viewed by clicking **User's Manual.**

6. Start Microscope

Connect your Microscope to your PC USB port, start the



software by clicking the MicroCapture Pro icon generated on the desktop after installation and you will see the following screen pop up.



When the Microscope is disconnected from your PC USB port, the following message will pop up.

No Device detected, please connect your Microscope directly to your PC USB port.

7. Software functions

■ Capture Photo



a. Click 'Photo' shortcut icon

in the main menu

bar.

b. Click 'Capture > Photo'.



■ Capture Video



a. Click 'Video' shortcut icon

in the main menu

bar.

b. Click 'Capture > Video'.




■ Timer (Photo / Video)



Click 'Timer' shortcut icon

in the main menu bar.




- * Under Timer photo, you can set the start time, interval time and total picture number.
- * Under Timer video, you can set the start time, interval time and total video number.

Calibration and Measurement

Please make calibration before measurement.

Calibration

Display Crossing from 'Options>Crossing".

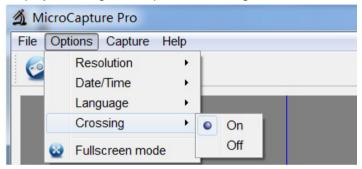


Microscope default at crossing "on"

It's used to check the dial on the calibration ruler.

1. Focus microscope on the attached calibration ruler

and then adjust the magnification till the picture is clear. Take a picture for the selected area when the dial is parallel to the crossing as below.



2. Double-click on the picture to enter into measurement interface as below.



3. Click Calibration icon, and then move mouse to the picture. Click on the beginning and ending points across a known value. Now a dialog will popup as below and you need to enter the exact value of the measurement sample into 'Actual dimension'.


Then the software will automatically calibrate the magnification rate. Click 'OK' and the adjusted magnification rate will show in the upper right corner.



^{*} Remark: The measured line should be paralleled.

4. Now you can use 'Any angle Line' under Measurement

icon to measure the value again. If the value you measure by software is nearly the same as the exact value of the dial means the calibration finish.

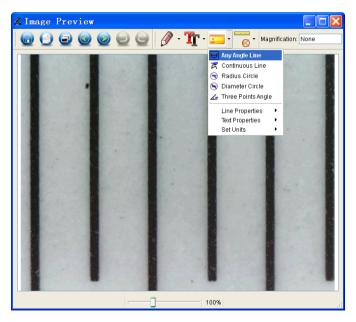

Measurement

Double-click on the picture to enter into measurement interface. Under the 'Measurement' icon , you can choose any desired options to measure.

- 1. Any Angle Line Measurement
 Simply click from one point and drag to the next point, and
 then release the click.
- Continuous Line Measurement
 The Continuous Line measurement allows you to measure any continuous desired length.
 Simply click and drag from one point to other desired points, and then release the click.
- Radius Circle Measurement
 Simply click and extend out to the desired radius, the radius, circumference and area of the circle will show up accordingly.
- 4. Diameter Circle Measurement Simply click and extend out to the desired diameter, the diameter, circumference and area of the circle will show up accordingly.
- 5. Three Points Angle Measurement Simply define any three points angle and click, the angle value will then display.


Change Calibration

If you need to change the magnification rate and adjust focus to capture picture, please calibrate the magnification rate again.

1. Double click to open the picture, Click '




Reset magnification > Reset picture magnification' as below. And then start calibration again (Calibration details please refer to page 37).

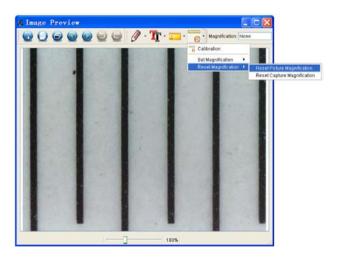

Change the magnification rate and capture several pictures, click on the picture to enter into measurement

interface. And click '_____> Set magnification > Set picture magnification', now a dialog will show up as below; enter the magnification rate into the dialog and click 'OK'.

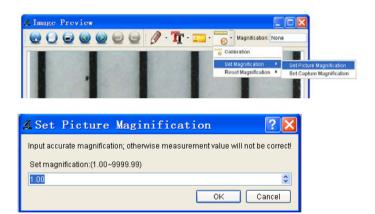

3. If you want to use the same magnification rate to

capture pictures, just click ' > Set
magnification >Set capture magnification'. Now all
pictures will use the same magnification rate and you can
start measurement directly.

handandan



Draw and Text

You can draw or add a text on the picture and save for later analysis.

1. Click icon to choose any kinds of drawing under the pull-down manual as below.



2. Click icon and set the font for the text in the popup dialogue as below.



8. Software Interface Instructions

Main Interface Icons



Capture photo – It's used to capture photo one by one.



Start / Stop record video.



Timer for photo / video – Set the start time, interval time and total photo/video number.




Full screen mode,

Press ESC or double-click to exit.

Main Menu

File

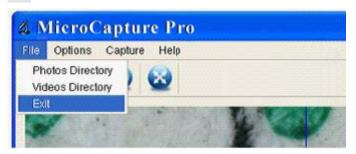


Photos Directory: set the directory to store photos

taken;

Videos Directory: set the directory to store video taken;

Options

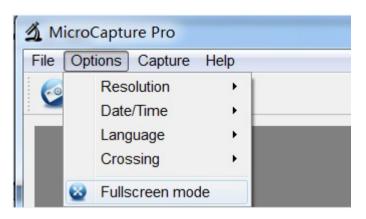

Resolution: change preview size

Date/Time: set to display system date/time on preview

window

Language: choose different OSD language

Crossing: display cross on preview window

Fullscreen mode: enter into full screen. Click ESC or

double click to exit

Capture

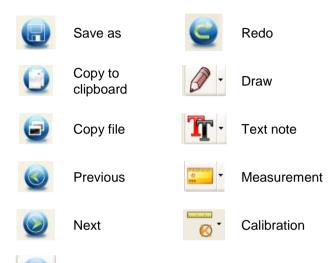


Photo: take a photo

Video: record a video clip

Measurement Interface Instructions

Undo



Instructions for Mac software

Part I How to Install the Software

Open *mac* folder from the disc and copy **MicroCapture Pro** onto your desktop for daily use.



Part II How to use MicroCapture Pro


- 1. Plug Microscope into PC USB port.
- Double click MicroCapture Pro icon to open the MicroCapture Pro window. The microscope is now ready to use.



MicroCapture Pro

3. Preview

At the central window, you can preview the magnified subject.

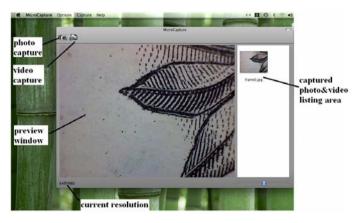

4. Change preview resolution


From *Options*, you can choose the preview resolution. The current resolution will be displayed at the left bottom corner of the preview window.



Please note that the preview window size always remains at 640x480 but the current resolution will show at the left bottom corner.

5. Date/Time


From Options, you can turn the date/time on or off.

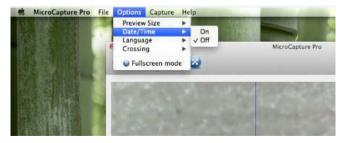

6. Photo capture

You can capture photo by:

• Choosing Capture/Photo

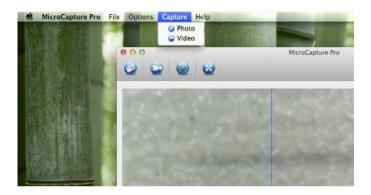

clicking photo capture icon



The captured photos will appear as thumbnails on the right side of the preview window.

7. Video capture

You can capture video by:

1) choosing Capture/Video



2) clicking video capture icon




Note: After clicking on the icon, the video capture icon will turn red to indicate video clip recording. Click the red icon again, to stop recording!!

The captured videos will be appearing as thumbnails on the right side of the preview window under Video tab.


8. Photo & Video editing

Captured photo & video appear as thumbnails on the right side of the preview window.



1) Photo

Double click a photo thumbnail to open in the main preview window



You can then carry out operations as you normally do on Mac system.

2) Video

Click a video clip thumbnail, the video will play automatically.

9. Quit MicroCapture

Choose **Quit MicroCapture** as follows, you can quit the software.



EN

This symbol on the product or in the instructions means that your electrical and electronic equipment should be disposed at the end of its life separately from your household waste. There are separate collection systems for recycling in the EU. For more information, please contact the local authority or your retailer where you purchased the product.

